


**Supplemental Figure S11.** Network meta-analysis for Breathing problems of each device.

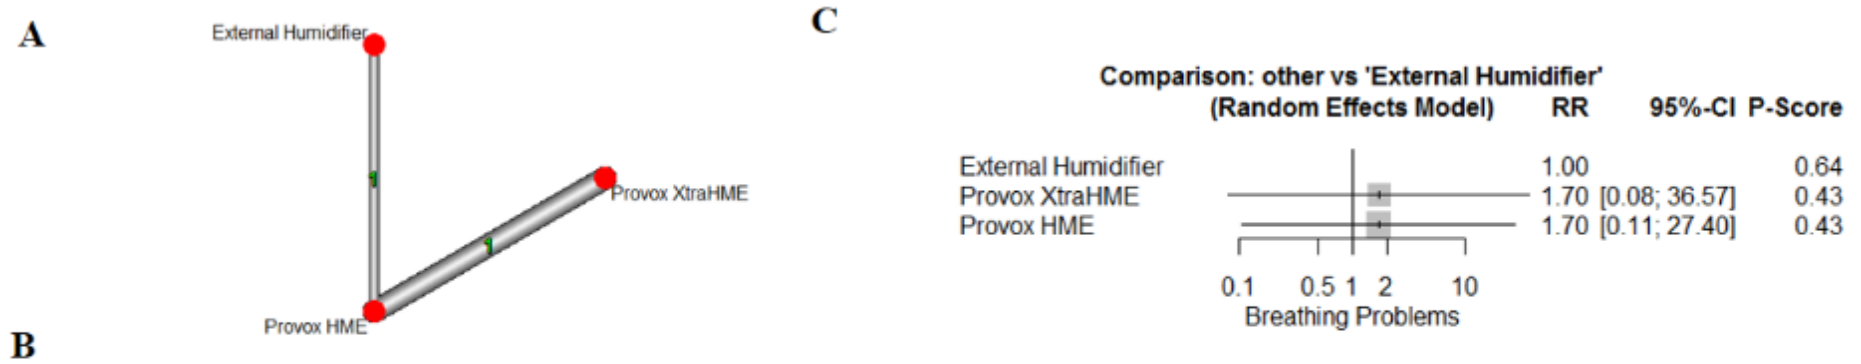

<b>External Humidifier</b>		
<b>0.59 [0.03; 12.61]</b>	<b>Provox XtraHME</b>	
<b>0.59 [0.04; 9.45]</b>	<b>1.00 [0.27; 3.67]</b>	<b>Provox HME</b>