

INITIAL SITUATION

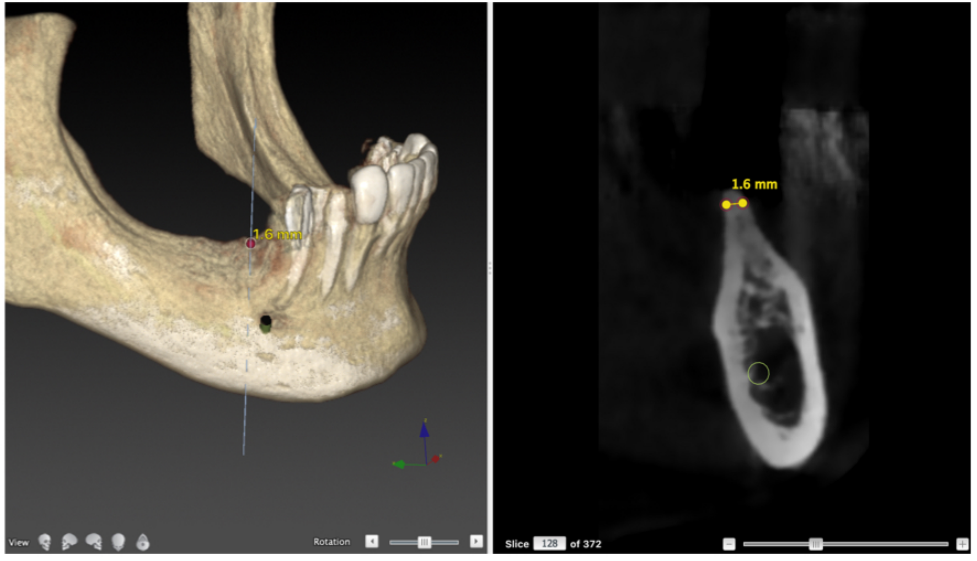


4.6

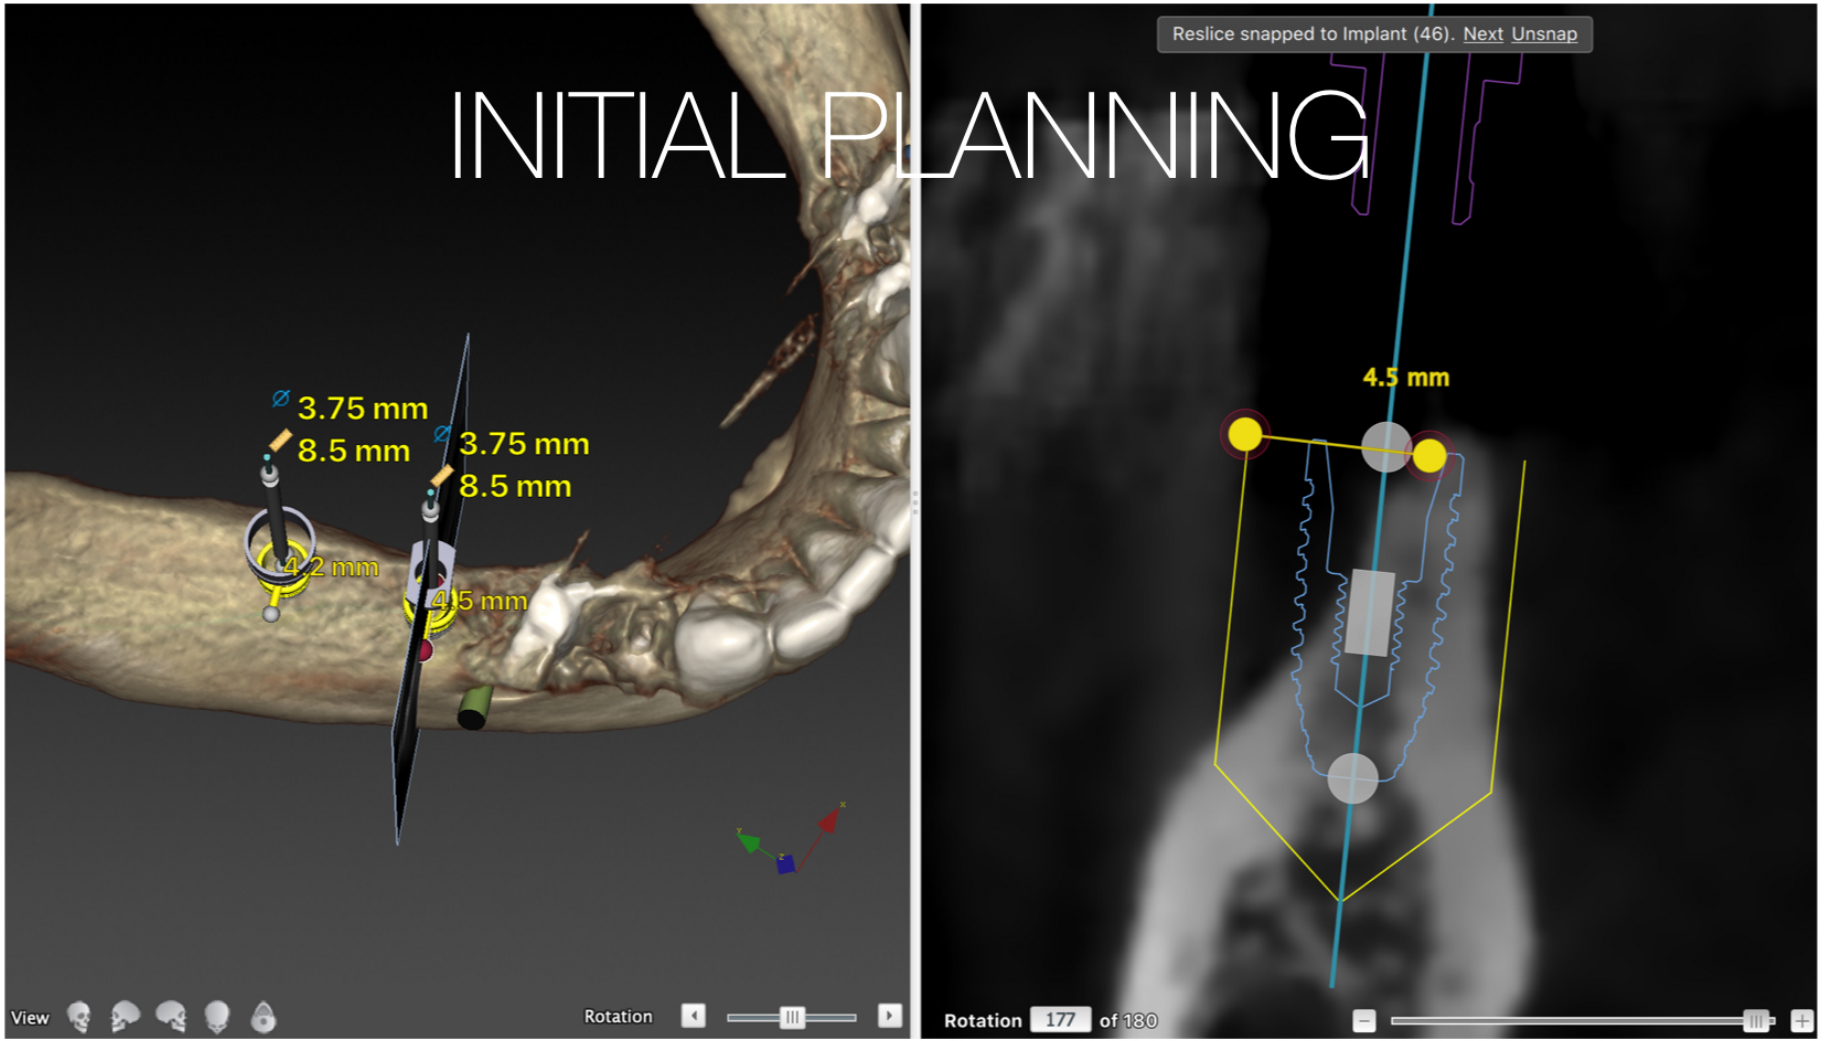



4.7



INITIAL PLANNING
3.75 mm
8.5 mm
3.75 mm
8.5 mm
4.2 mm
4.5 mm
View
Rotation
Reslice snapped to Implant (46). Next Unsnap
4.5 mm
Rotation 177 of 180

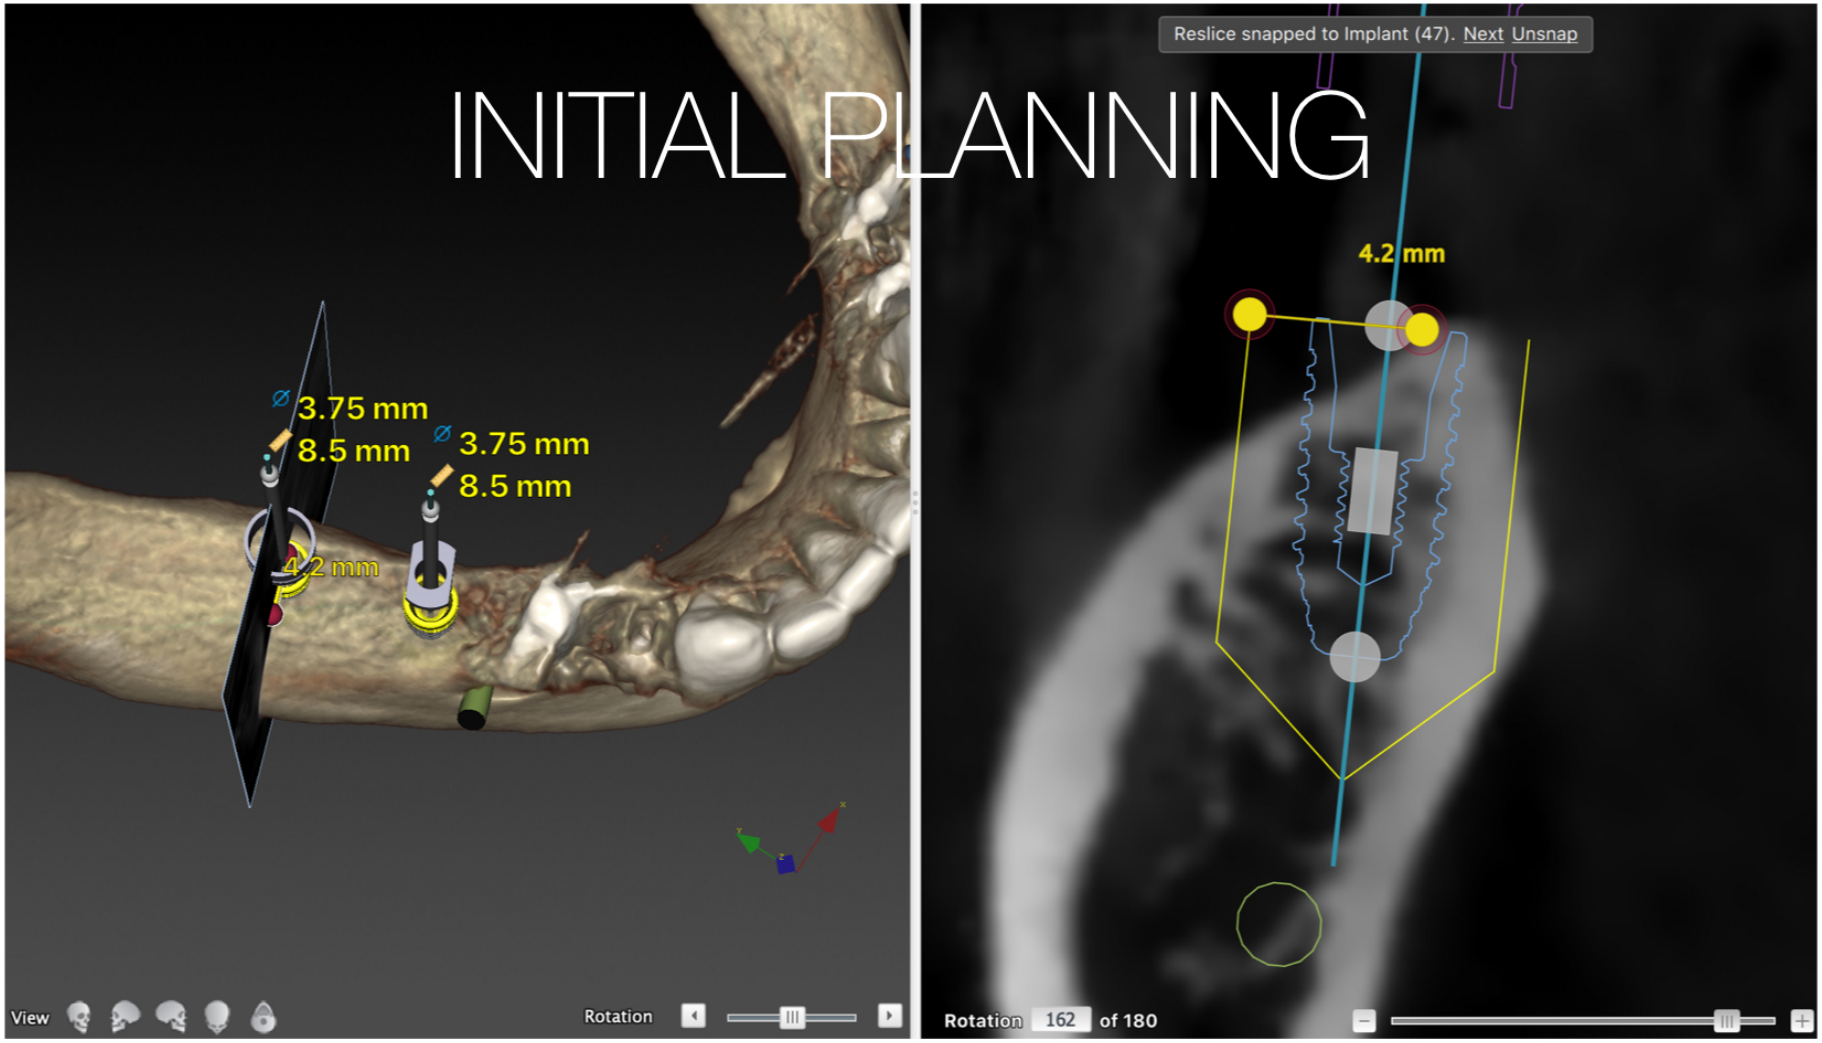
INITIAL PLANNING
3.75 mm
8.5 mm
3.75 mm
8.5 mm
4.2 mm
View
Rotation
Reslice snapped to Implant (47). Next Unsnap
4.2 mm
Rotation 162 of 180

INITIAL PLANNING

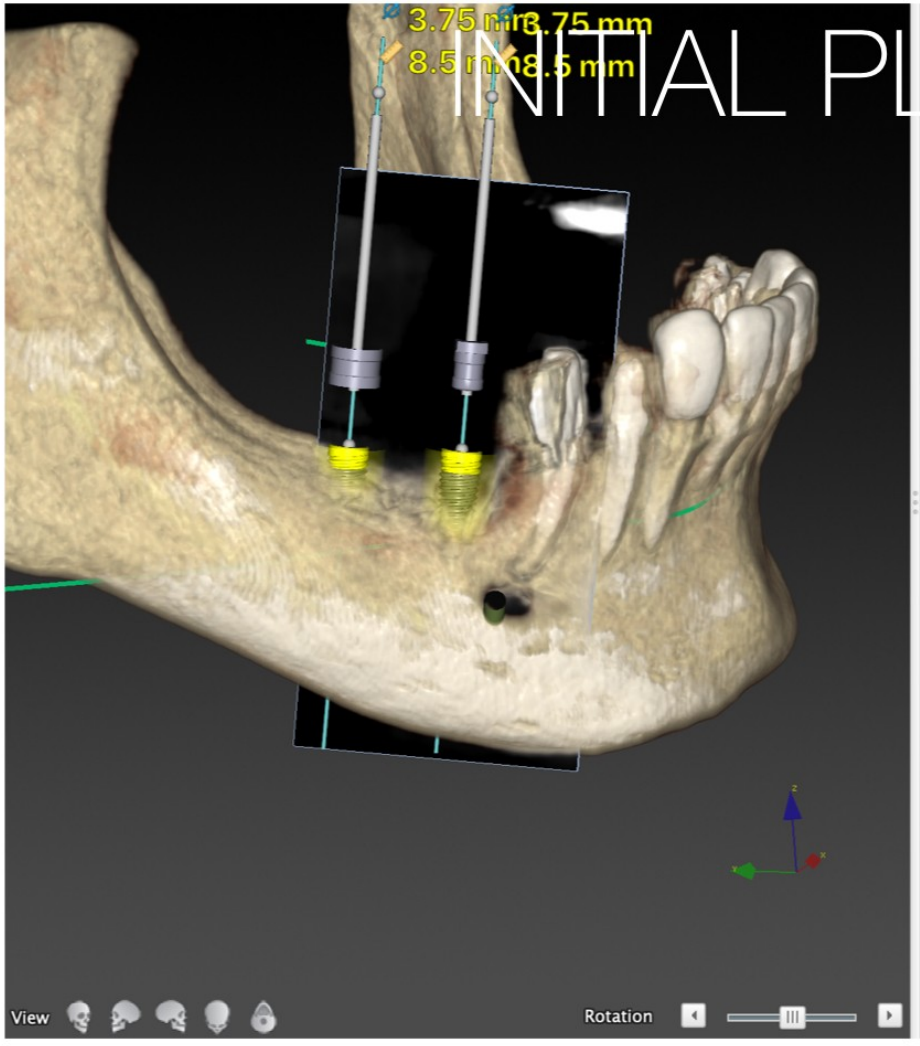

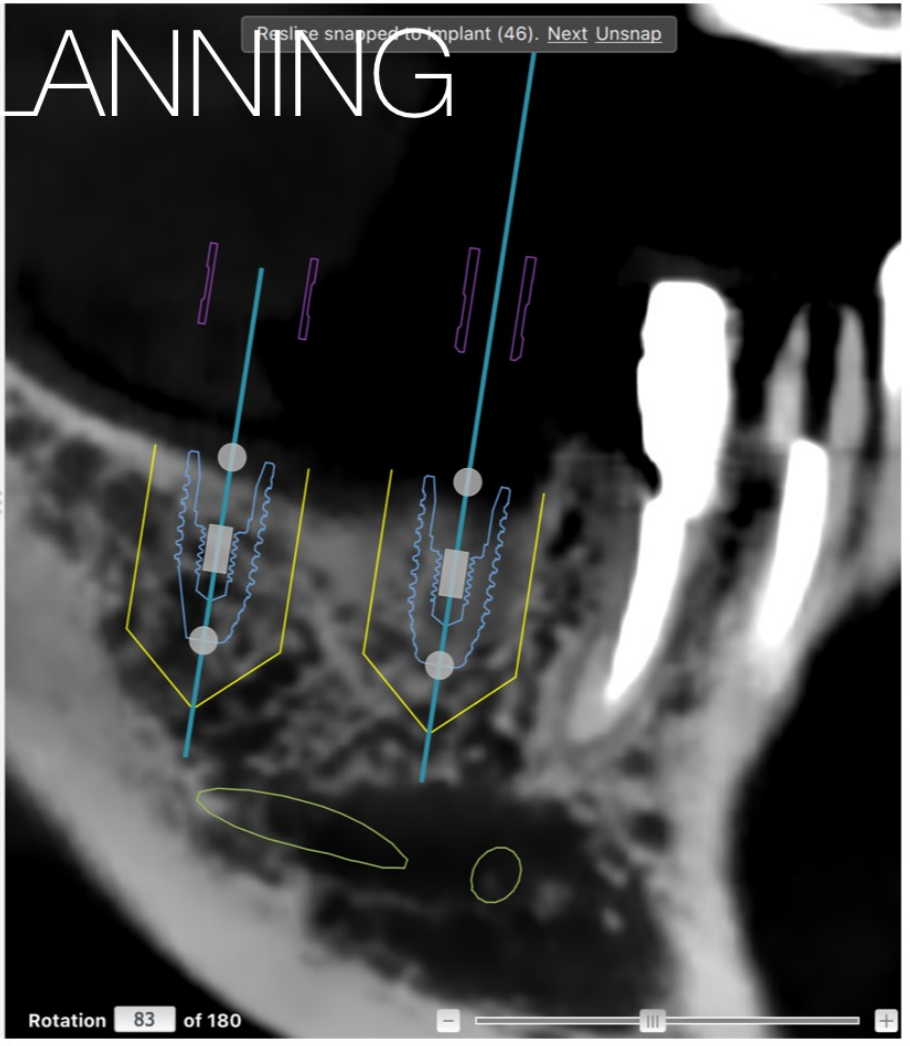

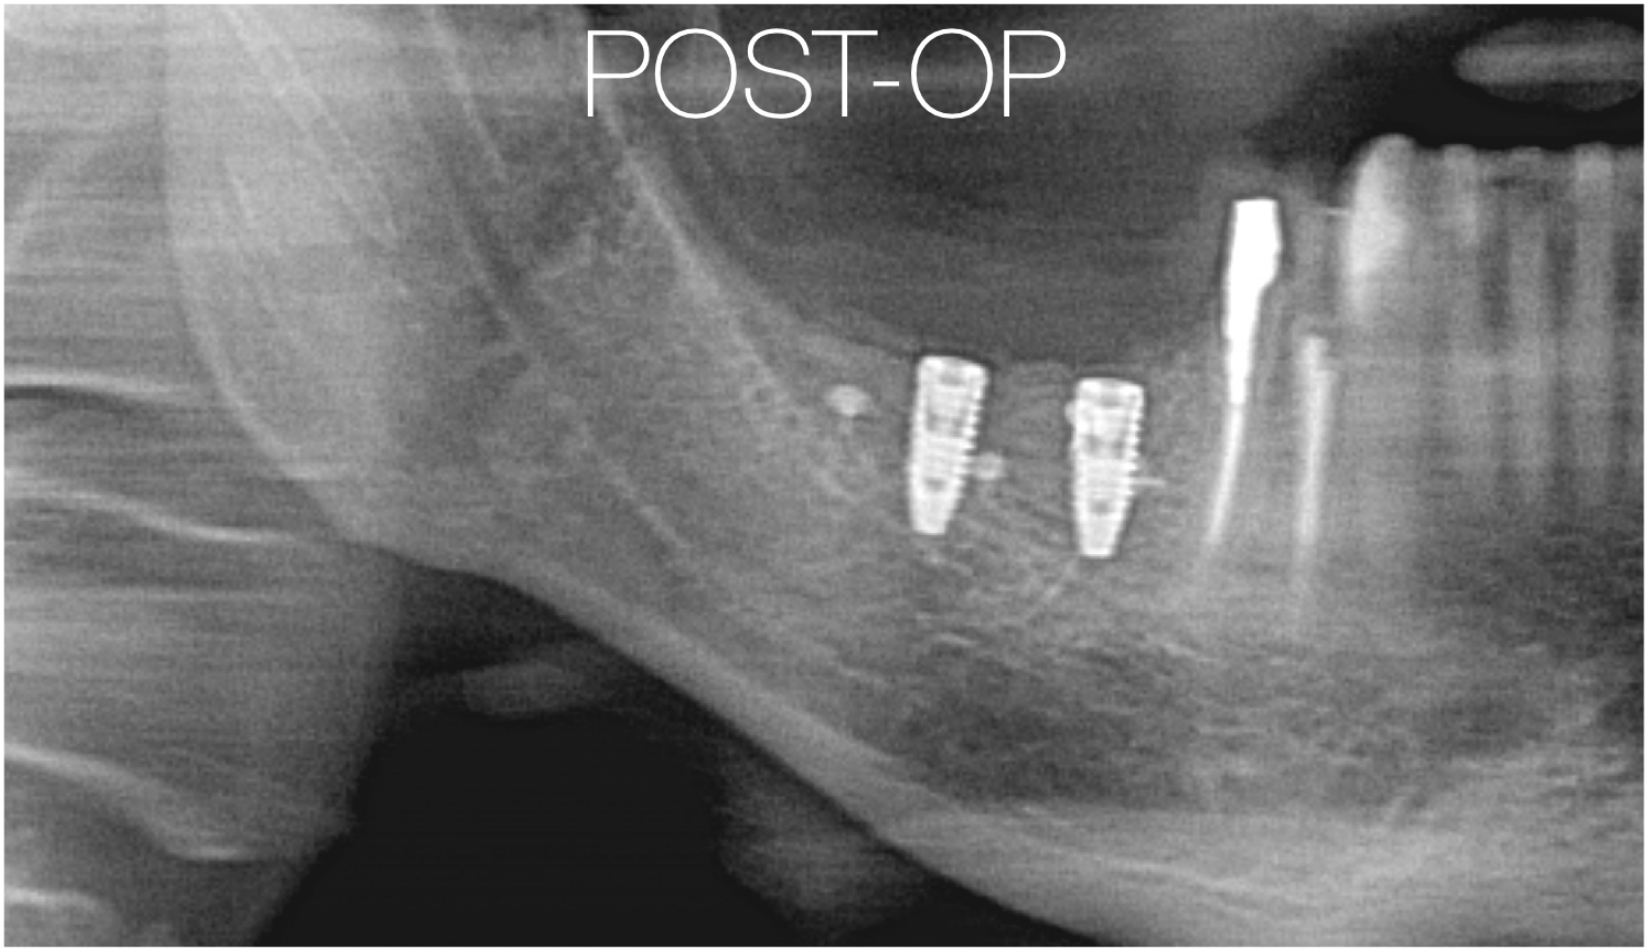
POST-OP